



IIIG03N005		A		REVISIONS	
ZONE	REV	DESCRIPTION	DATE	APPROVED	

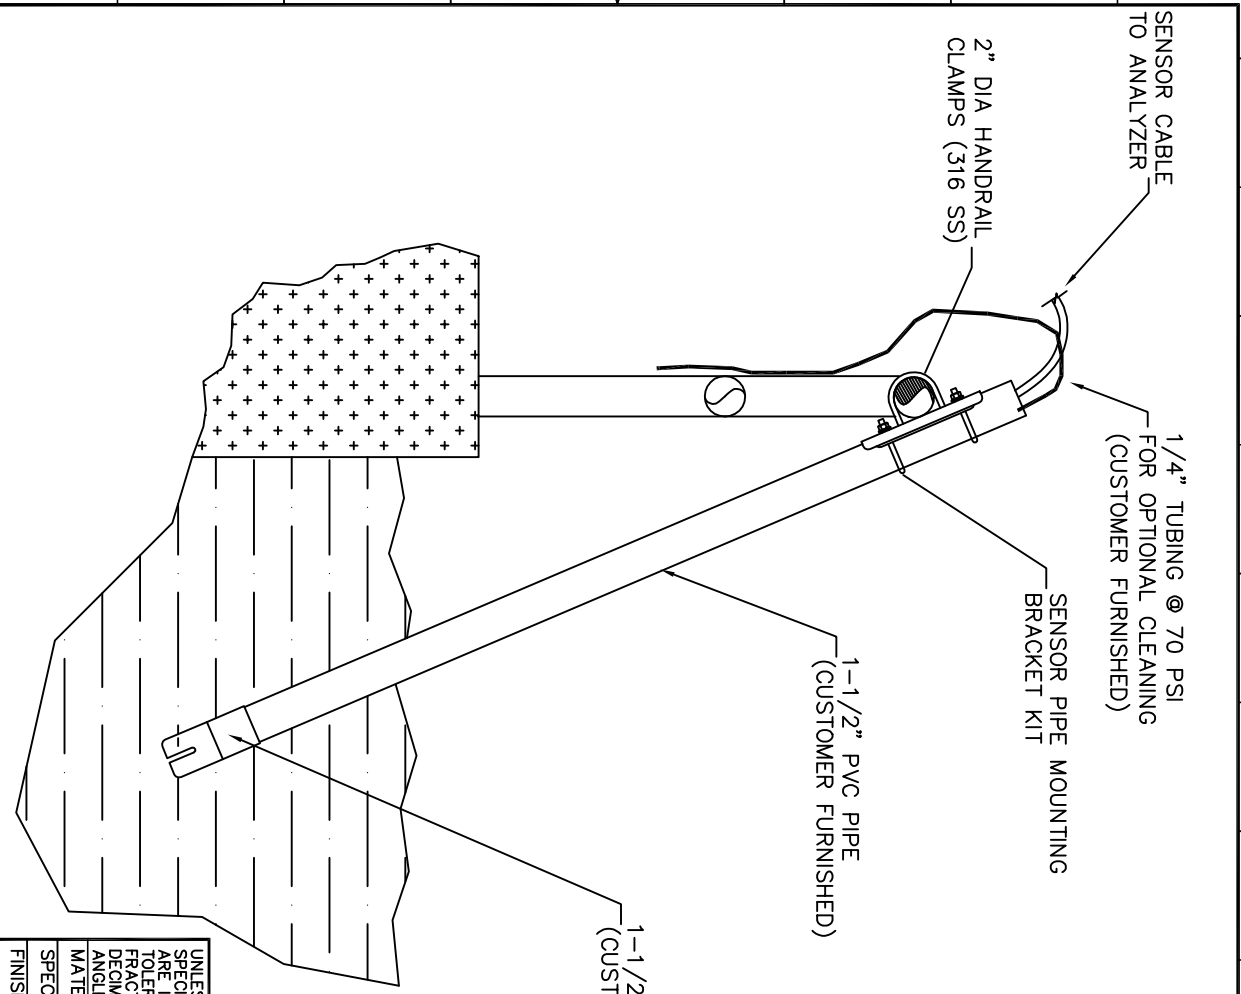

- Notes:
- 1) Material: Epoxy, Polyurethane, & PVC
 - 2) For best accuracy, Suspended Solids measurements should be taken 2ft. below the surface and 3ft. from the wall.

UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN INCHES. TOLERANCES ON: FRACTIONS DECIMALS ANGLES MATERIAL SPEC FINISH		CONTRACT NO.		 80 Whisperwood Blvd. Suite 107 Slidell, LA 70458	
SIGNATURES	DATES	SIZE	FSCM NO.	DRAWING NO.	REV
DRAFTSMAN		B		IIIG03N005	A
CHECKER		SCALE			
DESIGNER		NTS			
PROJ. ENGR.					
RELEASED					
APPROVAL					

TSS SENSOR MOUNTING