


REVISIONS		DATE	APPROVED
ZONE LTR	DESCRIPTION		

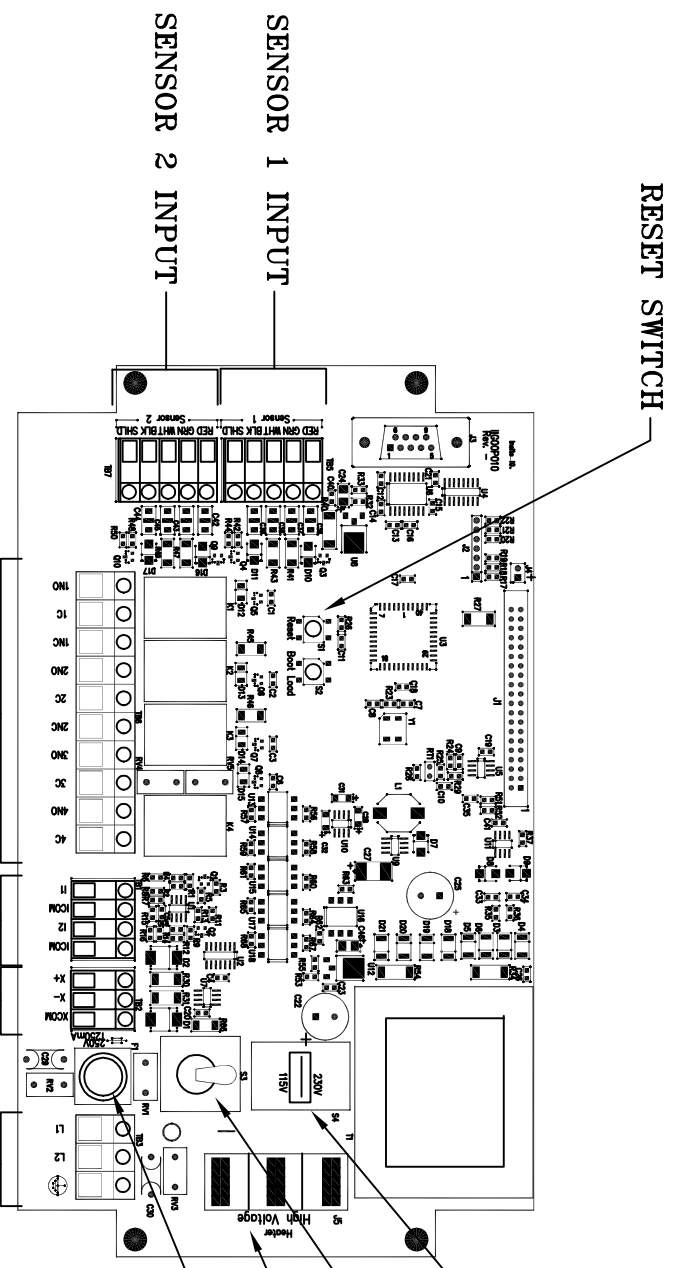

**!** Circuit Breaker meeting IEC-947-3 must be on line supply, in close proximity to equipment and shall be marked as the disconnecting device for the equipment.

**!** 115 OR 230 VAC @ 50 OR 60 HZ MAIN POWER CONNECTION AND WILL NORMALLY CONSUME LESS THAN 25 WATTS.

MODBUS INTERFACE (RS-485)

ANALOG OUTPUT (0-20 or 4-20ma) 600 OHMS MAX. LOAD

UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN INCHES		CONTRACT NO.	
TOLERANCES	ANGULAR	DRAWN	DATE
DECIMALS .XX ±.010	X' ±.1"	CHECK	
.XXX ±.005		D. RADLE	
DO NOT SCALE DRAWING		DESIGN	
MATERIAL		APPROVED	
FINISH		D. RADLE	
SPEC.		CUSTOMER	
TITLE		SIZE	DWG NO.
CUSTOMER CONNECTION		C	IIG04R111
INSITE IG ANALYZER		SCALE	NTS
80 Whisperwood Blvd. Suite 107 Slidell, LA 70458		SHEET 1 OF 2	